

mectron

medical technology

# Инструкция по эксплуатации и уходу за аппаратом

## combi s



CE  
0476

1.0. –	.....	2
1.1. –	.....	2
1.2. –	.....	2
1.3. –	.....	3
1.4. –	.....	3
2.0. –	.....	5
2.1. –	.....	5
2.2. –	.....	5
2.3. –	.....	5
3.0. –	.....	5
3.1. –	.....	5
4.0. –	.....	5
4.1. –	.....	5
4.2. –	.....	6
5.0.–	.....	7
5.1.–	.....	7
5.2.–	.....	.7
6.0.–	.....	8
6.1.–	.....	8
6.2.–	.....	8
6.3.–	– .....	9
6.4.–	– .....	10
6.5.–	.....	12
7.0.–	, , .....	12
7.1.–	.....	12
7.2.–	.....	13
7.3.–	.....	13
7.4.–	.....	14
7.5.–	.....	14
7.6.–	.....	15
7.7.–	.....	15
7.8.–	.....	.15
8.0.–	.....	16
8.1.–	.....	16
8.2.–	.....	16
8.3.–	.....	17
8.4.–	.....	17
8.5.–	.....	17
9.0.–	.....	17
10.0. –	.....	18
11.0. –	.....	18
12.0. –	.....	18
13.0. –	.....	21
14.0. –	.....	23



1.3. –

• :  
 -  
 - , ,  
 -  
 -  
 -

• :  
 -  
 - :  
 -  
 -  
 -  
 -

1.4. –

Mectron

• :  
 1. .  
 2. .  
 3. , ,  
 4. , ,  
 5. « ».  
 :  
 , .  
 :  
 ( . 1.3.).  
 , , .  
 : , .  
 , , 5.0. , .  
 : , , , , .  
 , , «7.0».  
 :

Mectron

:

.

,

.

:

.

,

,

,

,

«

»,

.

:

,

.

-

,

.

.

.

:

.

,

,

.

,

:

.

,

,

.

:

.

/

/

,

(

/

).

,

150

:

.

.

,

,

,

.

:

,

(

,

..)


## 2.0.–

### 2.1. –

Mectron.

### 2.2.–

«13.0»)

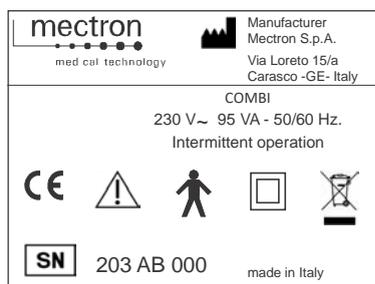

### 2.3.–



## 3.0.–

### 3.1. –

MECTRON,

## 4.0.–

### 4.1. –

MECTRON,



5.0.-

5.1. -

: , , .

: , .

: , .

: .

: .


: , , , , .

:

1. - 1-6 .
  2. , -
  3. 4-8 .
- :


5.2. -

- 1.
  - 2.
  3. ( ).
  4. ( ).
  5. ( ).
  6. ( ).
  7. ( ) . ( . 7.1.)
- Clean

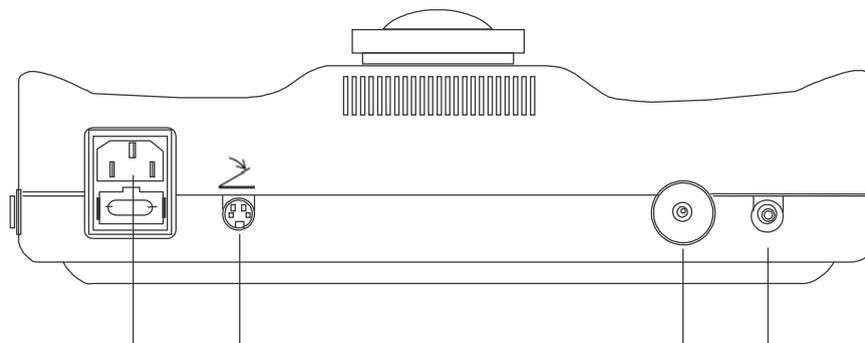

6.0.–

6.1. –

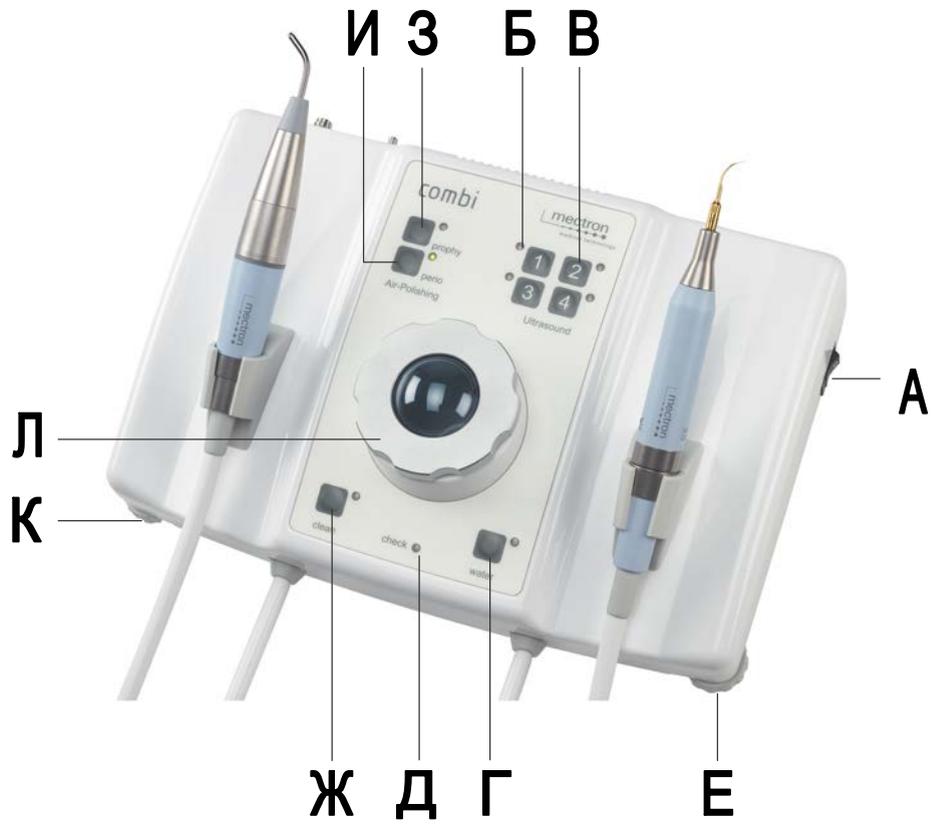

ON/OFF -

I/O

4

, , .

1-2-3-4

On/Off

:

–

Check

Clean

Prophy ( )

( - 150 )

Perio

, ( - 63 )

:

6.2. –

On/Off

I

:

On/Off

6.3. –

–

:

:

, , . . .

:

, , , . . .

:

/ /

/ ).

:

. , , , . . .

:

, , 7.0. , ,

:

, , , . . .

:

, , , . . .

- 1.0.
- 2.0.
- 3.0.
- 4.0.
- 5.0.
- 6.0.
- 7.0.
- 8.0.
- 9.0.
- 10.0.

Prophy ( ), (Perio Prophy)

On/Off ( I)

- 1.
- 2.

6.4. –

Mectron).

« Mectron. » (

«7.6 – 7.7 – 7.8».

( )

( ),

2

:

:

:

;

;

:

;

;

;

«

».

1.

2.

3.

( . 11)

:


:

;

;

(

)

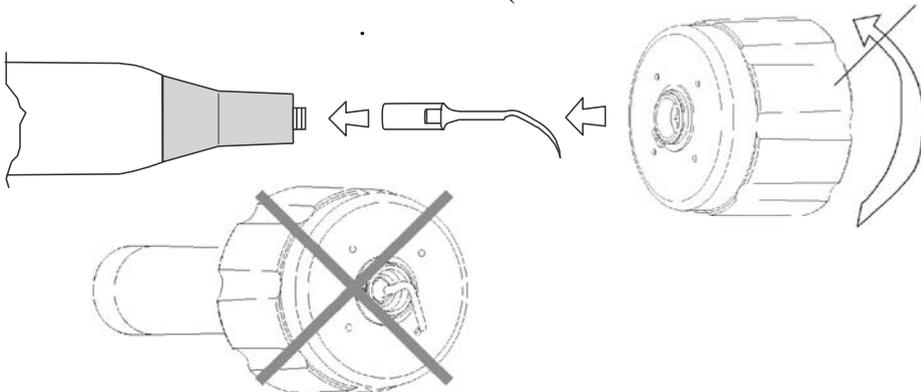

4. ( ).

**Ultrasound**

5. Water ( ).

6. ,

7. Water ( ).

8. ,

9. *pm* **Starlight**

**Starlight pm.** 2 4.

**6.5. –**

1.

2.

3.

4.

**7.0 –** ,

**7.1.–**

(Clean),

**Clean**

1. **Clean** ( )

2.

3.

4.

- 5  
- 13

5.

- 10 ..


;

7.2. -

- 1.
- 2.
- 3.

( 7).

7.3. -

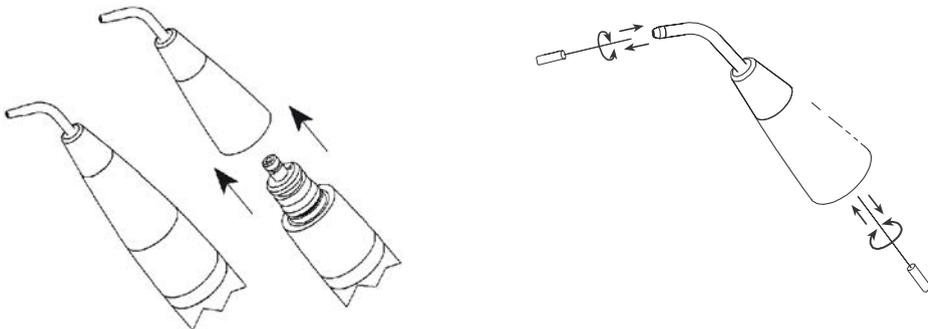

- 1.
- 2.
- 3.

:  
pH (pH7).

( 7).

( , , ).

#### 7.4. –

:  
**135°** **20**  
( . )

( , , , , )

: ,

,  
:

- 1.
- 2.
- 3.
- 4.
- 5.

#### 7.5. –

- 1.
- 2.

8.

3.

2%

:

4.

5.

6.


135°

20

:

7.6. –

- 1. , : .
- 2. : .
- 3. : .
- 4. : , .
- 5. ( ) .
- 6. 135° 20 .




7.7. –

- 1. ( ) .
- 2. .
- 3. .
- 4. : .
- 5. 135° 20 .

7.8. –

- 1. .
- 2. .
- 3. , .
- 4. : 135° 20 .

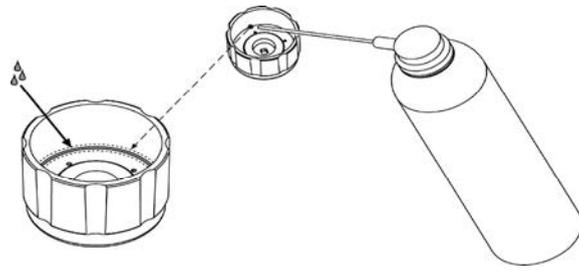

8. -

8.1.-

:

.

.

:

1.

2.

,

( )

3.

( )

,

,

4.


.

.

:

,

.

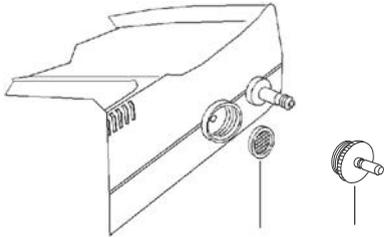

8.2 -

:

,

,

,


:

1.

( )

,

:

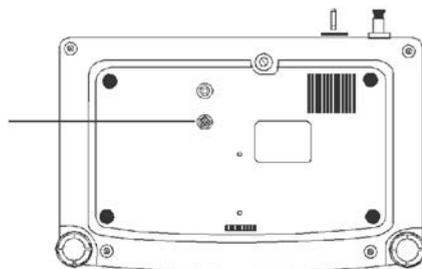

8.3 –

:  
.

,

8.4 –

:

- 1.
- 2.
- 3.
- 4.
- 5.
- 6.

( clean ( ), 7.1.  
8.2)

8.5. –

:

,

Mectron.

9.0.–

:

.

- 1.
- 2.
- 3.

( ).

:



,

:

- |      |          |
|------|----------|
| 230  | 500 mA T |
| 115B | 800 mA T |
| 100B | 800 mA T |

- 4.

( ).

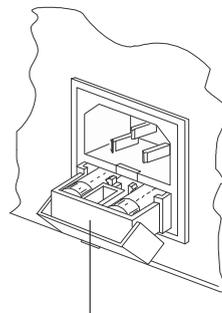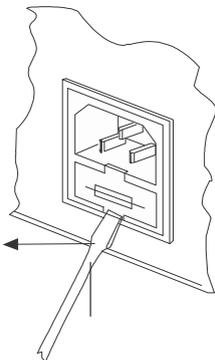

10.0. –

11.0. –

S1:

S2:

S3:

S4:

S5:

S1,

S6-S7-S8:

1- 2- 3- 4:

10- 11- 12- 13- 14:

R1-R2-R3-R4-R5:

D1-D2-D3-D4:

1- 2- 3- 4:

ER1-ER2-ER3-ER4-ER5:

1- 2:

12.0. –

		( 9.0.)
		MECTRON.
		7.5. MECTRON.
		7.5. 8.2. 6.3.) Mectron.

		7.5.
		8.1.
		8.3.
		( 4 8 ). ( . 6.3.). Mectron. 7.5. 8.2.
		MECTRON.  MECTRON.  MECTRON.
		<b>water</b>

		8.1.  MECTRON.
	( ). , ( ). ( ).	MECTRON.

**13.0. –**

**EEC Directive 93/42:**

II a

**EN 60601-1**

II

IP 20 ( )

IP 22 ( )

: .60 ,, .30  
.30 ,, .120 .

: 230 ±10% 50/60  
115 ±10% 50/60 ( )  
100 ±10% 50/60 ( )

: 66

: 5 20 .230 2 500 mA T  
5 20 .115 2 800 mA T  
5 20 .100 2 800 mA T

: 24 36

: 4 .

:

:

:

,

- . 7.1.

,

: 1 6 .

:

. 7.1.

,

, 4 8 .

:  
**Prophy – 3,5 , Perio – 2,7 .**

:

( )

:

, :  
« ».

:

+10° +40° .

:

30% 75%

:

-10° +70° .

:

10% 90%

: 500hPa/1060hPa

:

3,5 .

:

280 185 100 .

( )

14.-

MECTRON

MECTRON

, . . . , 2 ( ) , ,

MECTRON ( ) , ,

MECTRON

MECTRON ,

, / , , , , , ,

Bluelight s,

:

) 20 ( )

MECTRON ( )  
MECTRON

MECTRON

( )

a)

)

)

)

, MECTRON